Fig. 1A

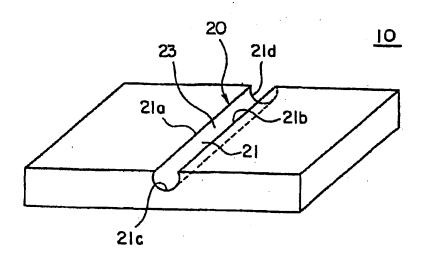


Fig. 1B

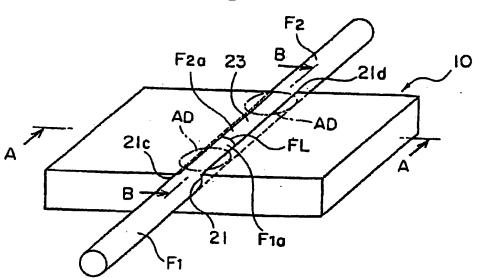


Fig. 2A

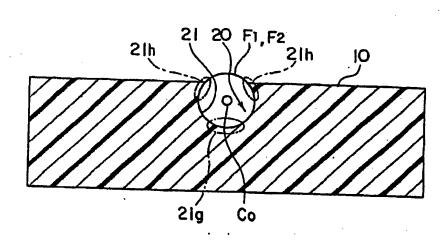


Fig. 2B

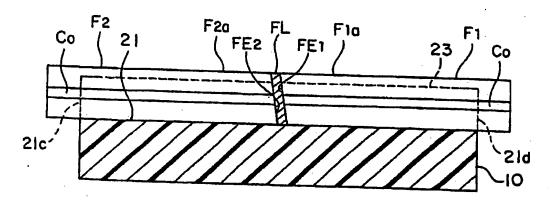


Fig. 3A

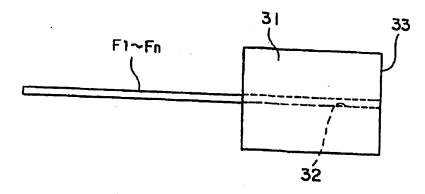


Fig. 3B




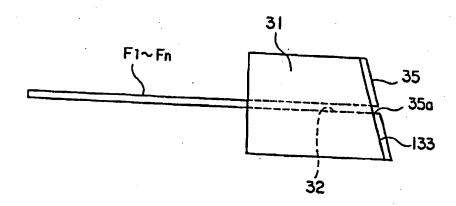


Fig. 3C

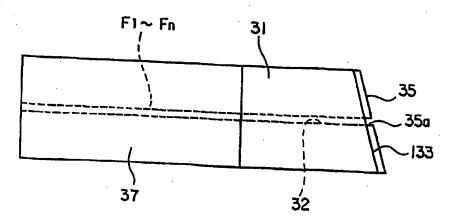

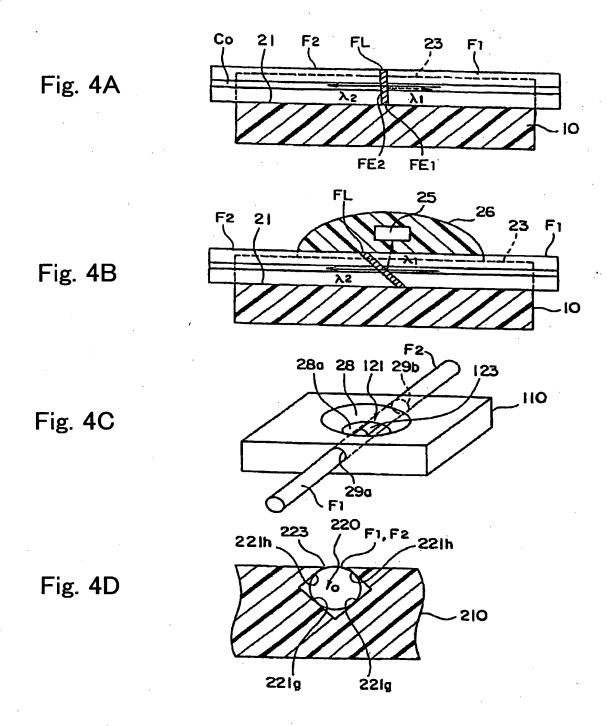

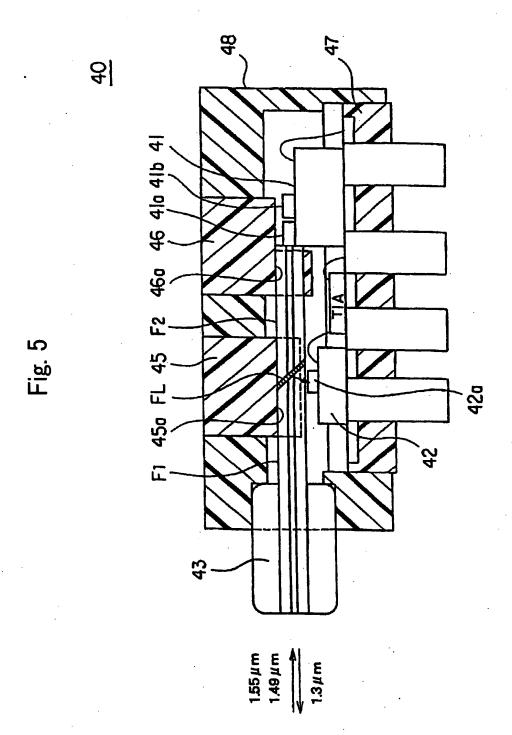

Rec'd PCT/PTO 13 APR 2006

OBLON ET AL (703) 413-3000:

DOCKET # 27045/WS SHEET 6 OF 16

Fig. 6

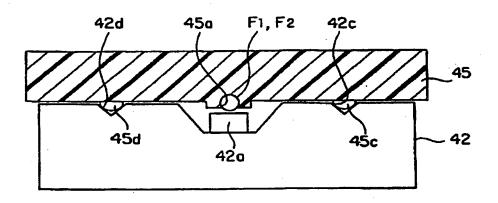


Fig. 7

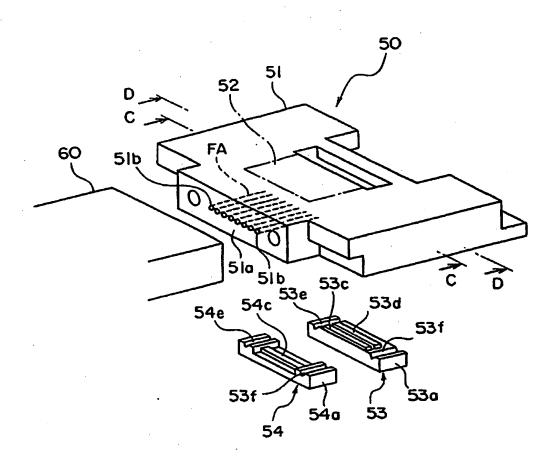


Fig. 8A

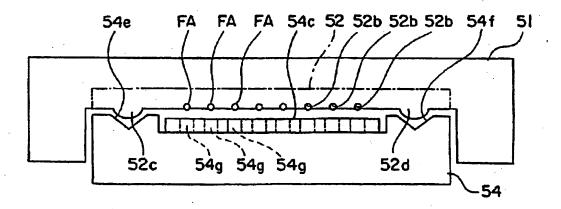
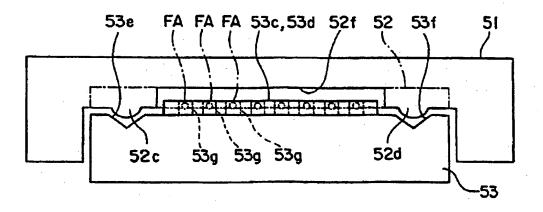
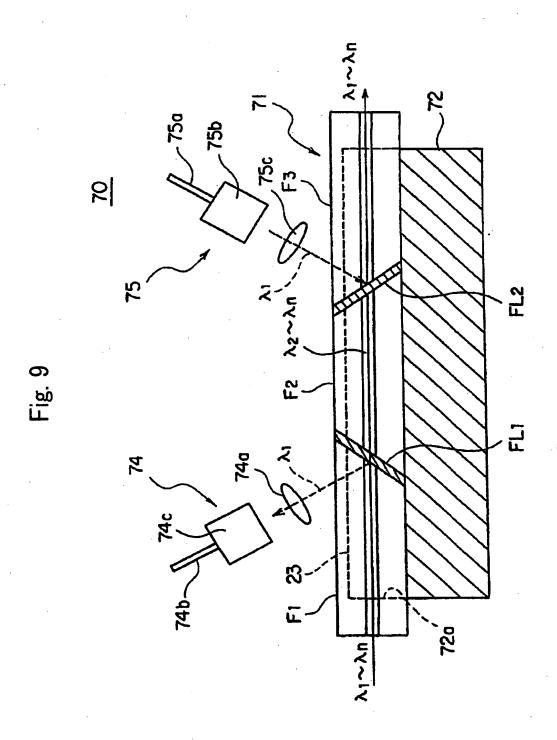


Fig. 8B





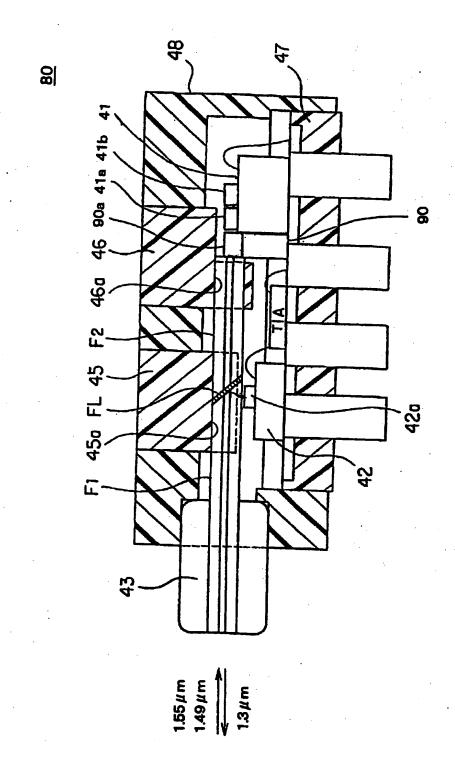


Fig. 10

Fig. 11

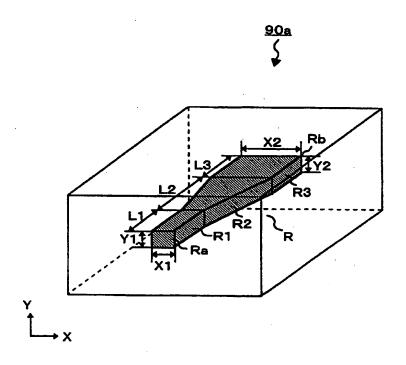


Fig. 12

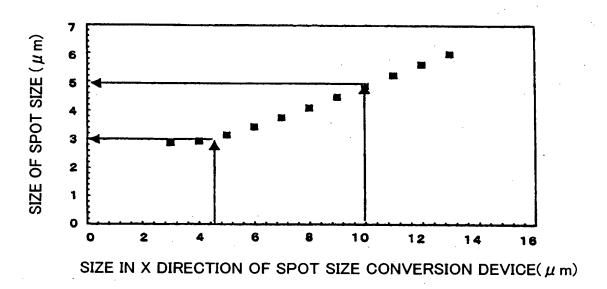
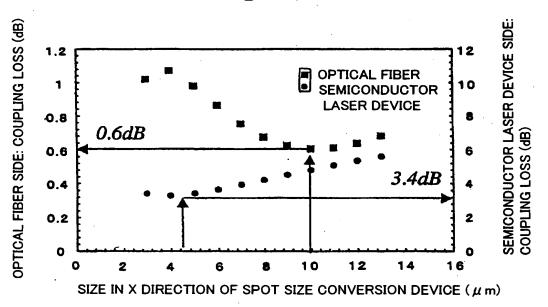


Fig. 13



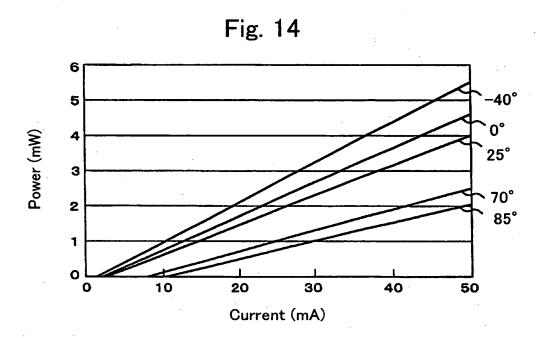


Fig. 15

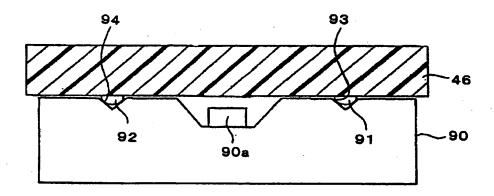


Fig. 16

